


## DOCUMENTATION OF QC ANALYSIS

Isoelectric Focusing (IEF) / Coomassie Blue Staining, according to SOP152

Run number: Phast9999

Broad pI Calibration kit, pI 3 – 9

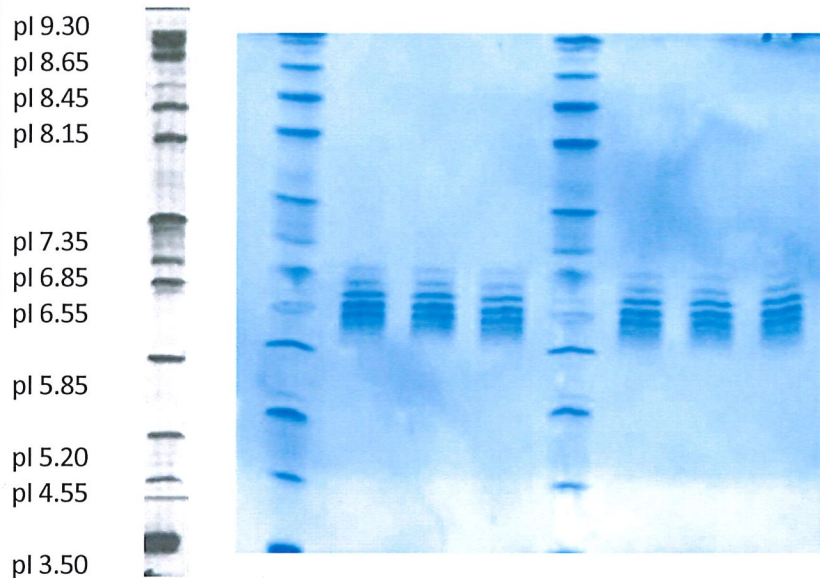

Lane	Batch number	Sample identification
1	ABC	Standard
2	Bxxxx	Sample A previous approved batch
3	Bxxxx	Sample B – 1
4	Bxxxx	Sample B – 2
5	ABC	Standard
6	Bxxxx	Sample C previous approved batch
7	Bxxxx	Sample D – 1
8	Bxxxx	Sample D – 2

Analysis performed date: 06.09.18

Signature: 