


## DOCUMENTATION OF QC ANALYSIS

SDS PAGE, stainfree, non-reducing, according to SOP166

Run number: SDS999

Precision Plus protein, unstained standard

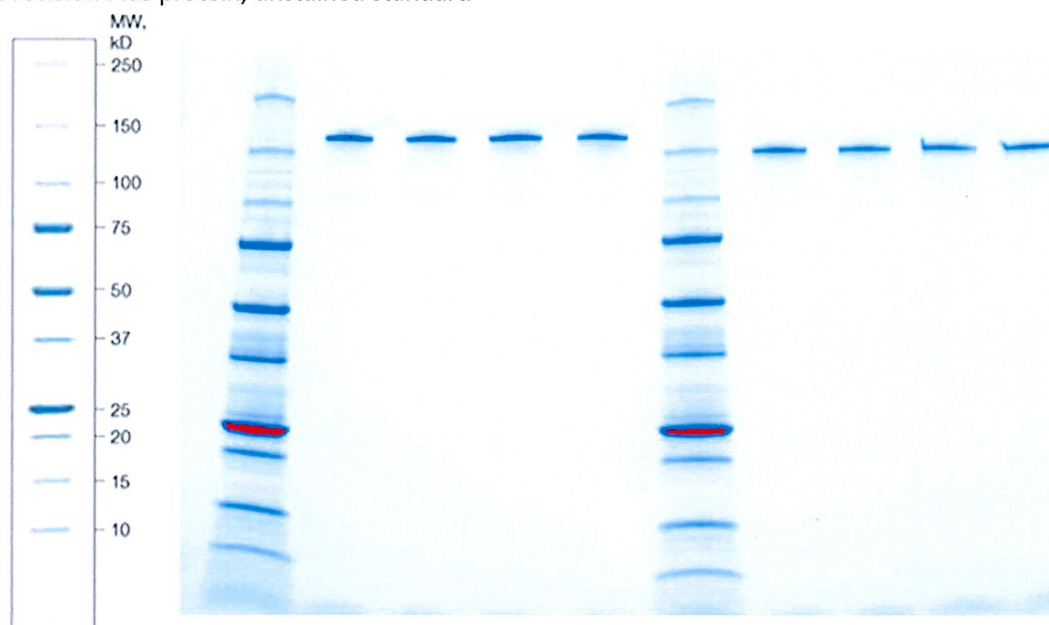

Lane	Batch number	Sample identification
1	ABCD	Standard
2	Bxxxx	Sample A – 1 previous approved batch
3	Bxxxx	Sample A – 2 previous approved batch
4	Bxxxx	Sample B – 1
5	Bxxxx	Sample B – 2
6	ABCD	Standard
7	Bxxxx	Sample C – 1 previous approved batch
8	Bxxxx	Sample C – 2 previous approved batch
9	Bxxxx	Sample D – 1
10	Bxxxx	Sample D – 2

Analysis performed date: 06.09.18

Signature: 